

Low Intensity Pulsed Ultrasound (LIPUS)

The application of ultrasound energy at much **lower** levels than is the current clinical norm is starting to gain ground as a therapeutic possibility. Clearly the applied energy is the same, it is the 'dose' which is different – most importantly, the intensity ($W\ cm^{-2}$) – which is **MUCH** lower – typically 2 or 3 times lower than the lowest setting on most regular clinical machines, with the most common application being at $30mW\ cm^{-2}$ (which is $0.03\ W\ cm^{-2}$).

At the present time, the strongest evidence for the clinical application of this modality is in relation to fracture healing, which is the area that this information sheet will concentrate on. It is argued – quite reasonably – that IF it works this well on bone lesions, then it should also be effective on other soft tissue lesions (ligament, tendon etc) but at the present time, the published research in this field is limited.


Examples of LIPUS devices available in the UK and Worldwide are illustrated below :

| | |
|--|--|
|  <p style="font-size: small;">EXOGEN is:</p> |  |
| <p>Exogen Device (Bioventus) (www.bioventusglobal.com)</p> | <p>Osteotron Device (www.itocoltd.com : www.emsphysio.co.uk)</p> |

LIPUS vs Regular Therapy Ultrasound

Ultrasound (US) is a form of **MECHANICAL** energy. Mechanical vibration at increasing frequencies is known as sound energy. The normal human sound range is from 16Hz to something approaching 15-20,000 Hz (in children and young adults). Beyond this upper limit, the mechanical vibration is known as **ULTRASOUND**. The frequencies used in therapy are typically between 1.0 and 3.0 MHz (1MHz = 1 million cycles per second).

Sound waves are **LONGITUDINAL** waves consisting of areas of **COMPRESSION** and **RAREFACTION**. Particles of a material, when exposed to a sound wave will oscillate about a fixed point rather than move with the wave itself. As the energy within the sound wave is passed to the material, it will cause oscillation of the particles of that material. Clearly any increase in the molecular

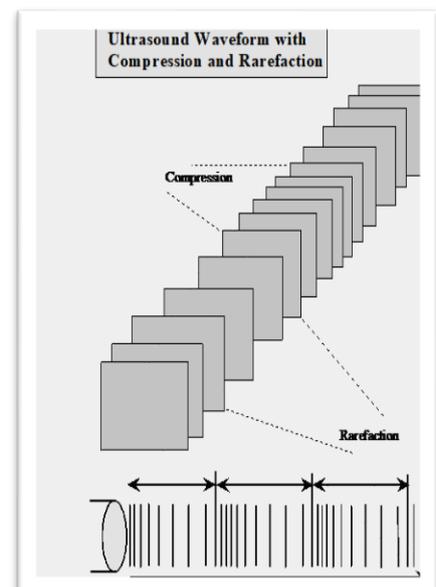

vibration in the tissue can result in heat generation, and ultrasound can be used to produce thermal changes in the tissues, though current usage in therapy does not focus on this phenomenon (Williams 1987, Baker et al 2001, ter Haar 1999, Nussbaum 1997, Watson 2000, 2008).

In addition to thermal changes, the vibration of the tissues appears to have effects which are generally considered to be '*non thermal*' in nature, though, as with other modalities (e.g. Pulsed Shortwave) there must be a thermal component however small.

Low Intensity Pulsed Ultrasound (LIPUS) is clearly ultrasound energy, but delivered at a much lower intensity ($W\ cm^{-2}$) than traditional ultrasound energy. There are other differences with the output of LIPUS devices, but this the most obvious issue.

Whilst a typical therapy machine will offer an operating frequency choice of 1MHz or 3MHz, the LIPUS fracture healing evidence has been generated almost exclusively at 1.5MHz. Both the Exogen and Osteotron devices offer LIPUS at this frequency, though the Osteotron device also offers a 0.75MHz (optional extra) probe which, it is suggested, would be effective for the more deep seated lesions (e.g. femur). No evidence has been identified for clinical trials with LIPUS at frequencies other than 1.5MHz, and therefore it is currently not known whether 'other' frequencies are effective, not as effective, or possibly more effective.

BNR - inequality of the Ultrasound Beam



As the beam emerges from the treatment head, the energy across the beam profile is not 'even' - there are areas of higher and areas a lower intensity. When the intensity is set on a therapy ultrasound device, it would certainly not be the case that every part of the beam, even as it emerges, would actually be at that intensity. The 'inequality' of the beam strength - or the 'beam unevenness' is represented by the Beam Nonuniformity Ratio (or BNR). In the ideal world this value would be, or be close to 1.0 (which means that there is equal power across the entire beam profile. In reality, most therapy ultrasound machines will have a typical BNR of between 4 and 6 (the smaller the better). If the

BNR has a value of 5 for example, it would mean that the 'strongest' parts of the beam would be at 5 x greater power than the mean power of the beam.

One of the reasons for needing to employ a 'moving treatment head' application technique is to

ensure that the 'strongest' parts of the beam are not always applied to the same part of the tissue - the treatment head movement helps to 'even out' the beam inequality.

A 'typical' beam plot can be seen in the diagram above and examples of 2 'real' beam X sectional plots from different transducers (at 3 MHz) from the Johns et al (2007) paper are illustrated (left) .

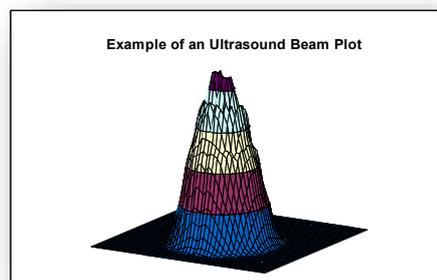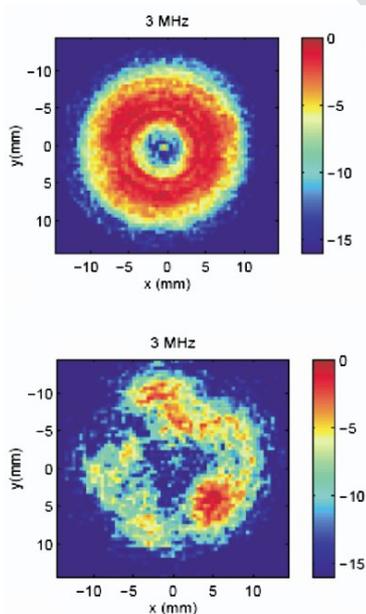

A recent analysis of clinical machines (Johns et al, 2007) identified that the BNR was in the range, 2.79-5.85 at 1 MHz and ranged from 2.51 to 4.56 for the 3.3MHz devices tested.

If (as with LIPUS treatments for fractures, the treatment head needs to be kept stationary for prolonged periods (typically 20 minutes), a LOW BNR is an essential safety issue.

The LIPUS devices for fracture healing have a low BNR - the Exogen being 4.0 (max) and the Osteotron being 3.0 or 3.5 depending on which applicator is employed.

Ultrasound Pulsing

Ultrasound on standard therapy machines can be delivered in a continuous or a pulsed mode, with pulse mode variations on many, if not all machines. LIPUS devices, having a narrow clinical application, tend not to offer such a wide range of pulse options.


Typical pulse ratios are 1:1 and 1:4 though others are available. In 1:1 mode, the machine offers an output for 2ms followed by 2ms rest. In 1:4 mode, the 2ms output is followed by an 8ms rest period. The adjacent diagram illustrates the effect of varying the pulse ratio.

Until recently, the pulse duration (the time during which the machine is on) was almost exclusively 2ms (2 thousandths of a second) with a variable off period. Some machines now offer a variable on time though whether this is of clinical significance has yet to be determined.

Some manufacturers describe their pulsing in terms of a percentage rather than a ratio (1:1 = 50% 1:4 = 20% etc). The pulse ratio - duty cycle percentage equivalence is shown in the table below:

| Mode | Pulse Ratio | Duty Cycle |
|------------|-------------|------------|
| Continuous | N/A | 100% |
| Pulsed | 1:1 | 50% |
| | 1:2 | 33% |
| | 1:3 | 25% |
| | 1:4 | 20% |
| | 1:9 | 10% |

LIPUS machines typically deliver their ultrasound pulsed at 20% (1:4) and at 1000Hz (1kHz) - therefore there are 1000 cycles per second, each cycle is thus 1/1000 of a second (i.e. a millisecond). In that millisecond, there will be 20% ultrasound and 80% not ultrasound. The ultrasound 'on' cycle will therefore be 0.2 milliseconds (200 microseconds or 200µs) followed by a 'gap' of 0.8 milliseconds (or 800 µs). The Osteotron device additionally offers a 100Hz pulse option.

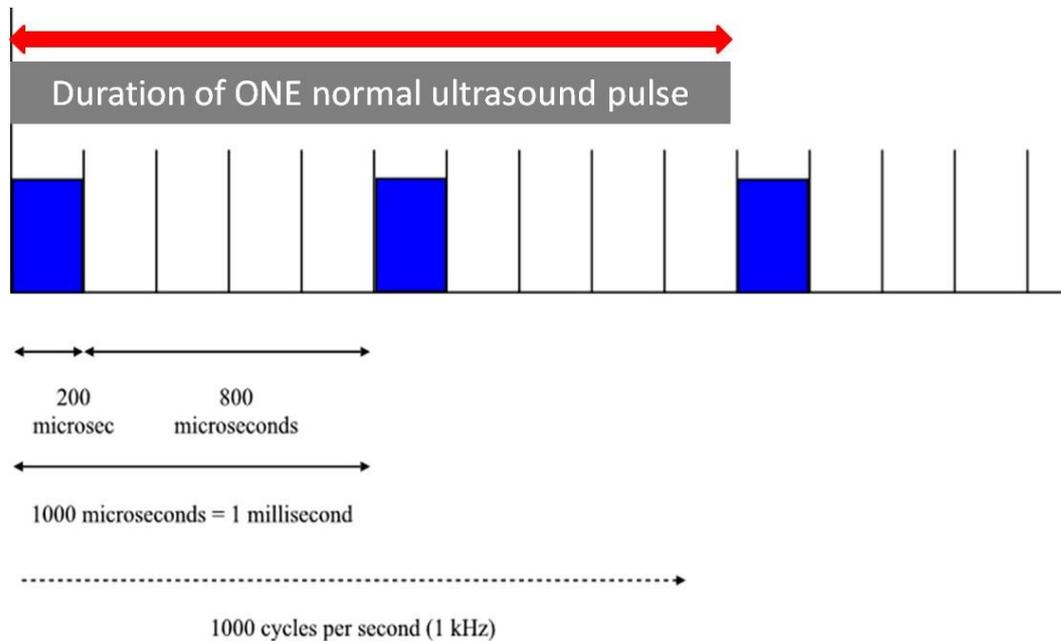

1kHz pulsing with LIPUS devices

Ultrasound Intensity

The intensity (strength in general terms - power density to be very specific) at which ultrasound is applied in regular clinical applications ranges from about 0.1 through to 1.0 W cm⁻². Some applications (researched and evidenced as being effective) will use intensities of up to 2.5 W cm⁻², and although not 'common' is certainly deemed to be a safe application mode and can be very effective in some clinical circumstances.

The power density clearly represents how much power is being applied (the Watts) and how concentrated it is (the cm²).

With the LIPUS devices for fracture healing applications, as mentioned in the introduction, one of the key differences is that the power density is much LOWER than with the traditional ultrasound treatments. Almost all of the LIPUS research has used 0.03 W cm⁻² (which is sometimes expressed as 30mW cm⁻²).


A typical therapy machine is not able to be set at power densities below 0.1 W cm⁻². It is not therefore known whether a standard therapy ultrasound machine can deliver a low enough 'dose' to be effective in this clinical area. At the moment, the available evidence would suggest that the sound energy that it delivers would be 'too strong' for the job in hand. Whilst there have been some (limited) animal experimentation (e.g. Warden et al 2006), this approach has yet to be formally evaluated in a human patient clinical trial.

The Exogen device (patient, take home, portable version) offers no power density options (it is always at 30mW cm⁻²) whereas the Osteotron device offers additional power options at 45 and 60 mW cm⁻² - though as far as the clinical evidence goes, none can be currently identified which supports the use of these higher dose options. It is suggested that they might / will be more effective for the deeper bone problems - which has logic, just lacks evidence at the present time.

A recent study by Fung et al (2012) (animal model - rat femoral fracture) set out to compare a 30mW cm⁻² and a 150mW cm⁻² treatment together with a control condition. The 30mW dose was shown to be clearly advantageous over both the 150mW and the control group recovery.

Ultrasound for Fracture Healing : Mechanism of Action

A considerable amount of research has been carried out to try and identify the mechanism by which LIPUS ultrasound applications can 'enhance' fracture repair. Necessarily, a high proportion of these studies are based on cell, lab and animal research, but they have served to provide an ever increasing picture of what is happening. It is suggested that this research area will continue to develop, and it is highly likely that additional information will continue to be published for some time to come yet - which will either add 'new pathways' to the existing ones or provide additional transduction or cytokine or gene expression data. It is appreciated that for many therapists, this is not the most important part of the 'story' and thus the following section will provide a summary rather than a fully explanation! Some of the key mechanisms identified in the research literature are illustrated in the figure below.

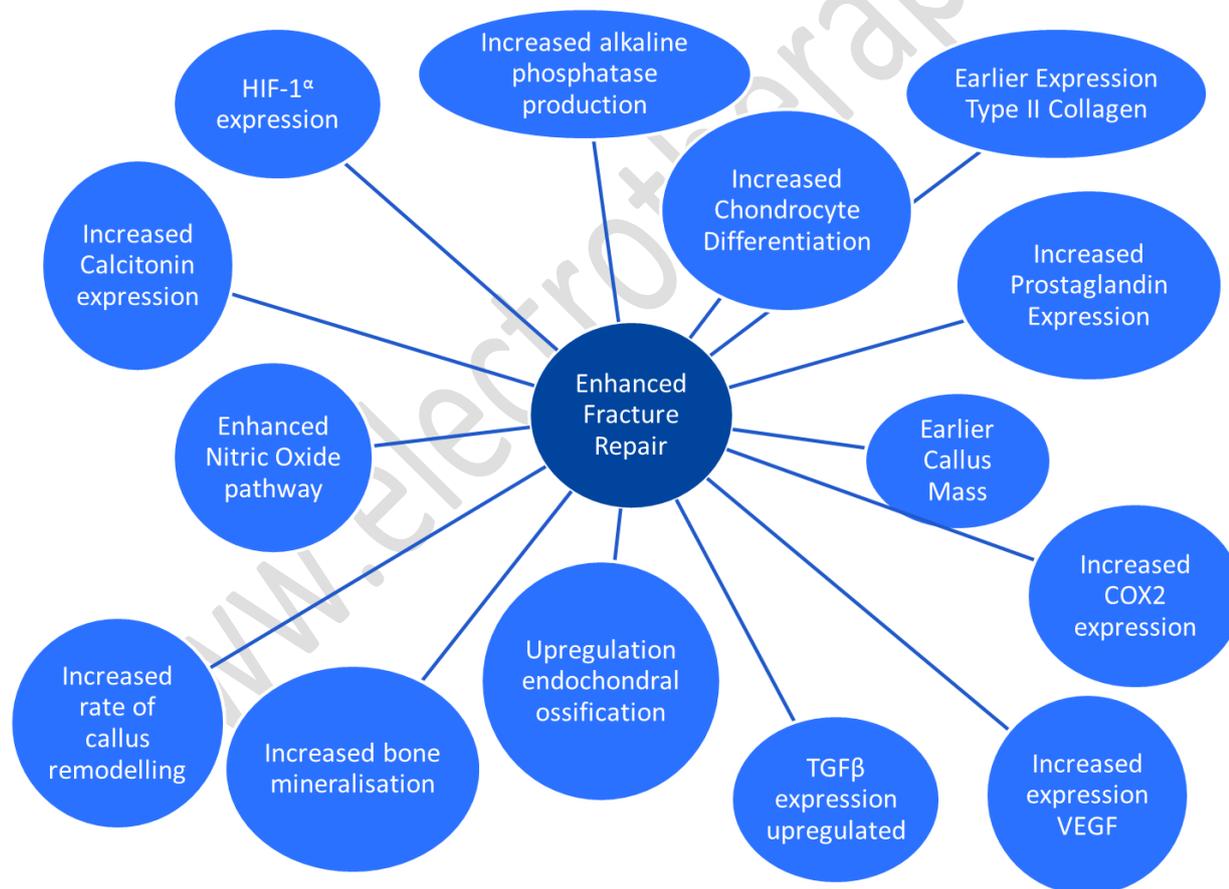

Useful summary and review papers can be found in : Claes and Willie (2007); Della Roca (2009); Jungushi (2009); Lu et al (2009); Padilla et al (2014) and Warden (2003).

The mechanisms which have been sufficiently well evidenced to justify their inclusion are listed below with some key references

Jungushi et al (2007) suggest that LIPUS is responsible for cell differentiation effects as a primary mechanism of effect rather than cellular upregulation or proliferation. They identify increased matrix

synthesis, earlier expression of Type II procollagen and also prostaglandin expression and an increased chondrocyte differentiation all being associated with LIPUS exposure. This results in an earlier callus mass, though not an increased (volume) of callus.

Other papers do appear to provide evidence for an increase in cell upregulation and proliferation. It is generally considered that the LIPUS energy has an effect at cell membrane level where mechanoreceptors (integrins) respond and result in various upregulation and expressions.

COX2 (Naruse et al, 2010) expression is increased. This is essential in the PGE2 pathway (it is necessary for PGE2 production), and both COX2 and PGE2 are known to be essential in fracture repair. Leung et al (2004) demonstrated increased expression of VEGF, a strong angiogenic stimulator and both Naruse et al (2010) and Sant Anna et al (2005) demonstrated increased expression of BMP2; BMP4; BMP6 and BMP7 (linked with TGF β) and linked to differentiation of stem cells (mesenchymal cells) into bone and cartilage. (BMP = Bone Morphogenic Protein).

There is an increased cell division in periosteal cells in the inflammatory stage (Leung et al, 2004) and in increased differentiation of chondrocytes triggered via a TGF β pathway (as above) (Ebisawa et al 2004). Upregulation of endochondral ossification (Kokubu et al, 1999, Sena et al, 2005) increased osteoblast differentiation (Lai et al, 2010), increased bone mineralisation (Leung et al, 2004) and increased rate of callus remodelling (Freeman et al 2009) have all been demonstrated as being associated with LIPUS exposure.

The Della Rocca (2009) review includes some additional information relating these and other gene expressions to the fracture healing pathway and the Padilla et al (2014) paper provides a useful overview of the evidence to date.

Other studies which contribute to the evidence base in this area include Nolte et al (2001) who identify an increase in ossification activity, Ryaby et al (1991) with increased TGF β synthesis. The increased expression of Type II collages from the chondrocytes is linked to a TGF β pathway (Mukai et al, 2005). The Kokubu et al (1999) study reiterates the essential contribution made by both COX2 and PGE2 to the fracture healing process. COX2 regulates PGE2 production, reinforced by the results obtained by Tang et al (2006). Both Reher et al (2002) and Warden et al (2001) identify NO and pGE2 pathways as being significantly involved in LIPUS fracture healing pathways.

This would be consistent with other proposed mechanisms of ultrasound action (ter Haar 1999) and the relationship between the use of NSAID's and tissue repair following injury.

Other elements described and identified include increased proliferation of periosteal cells, increased calcitonin expression, VEGF expression and alkaline phosphatase production (Leung et al, 2004). Wang et al (2004) argue that LIPUS exposure, resulting in increased VEGF, NO and HIF-1 α (hypoxia inducible factor 1 α) expression is an additional component of the stimulating pathway.

Without any further consideration of the detail of these mechanisms, it is clear that LIPUS energy, delivered to the fracture area results in an increased expression of several critical chemical mediators, growth factors and cytokines which have an essential role to play in the normal fracture healing sequence. It is evidenced that the LIPUS does not change the events of fracture repair but rather increases the expression of these various factors, and thereby stimulates the normal sequence. The resulting increased production of collagen, differentiation of cell types and change in callus production appears therefore to be a secondary effect as a result of the expression and upregulation functions.

Ultrasound for Fracture Healing : Clinical Issues

Numerous recent papers have identified the benefits of using therapeutic ultrasound for both normally healing (fresh) fractures and those that demonstrate either a delayed union or non union (e.g. Mayr et al 2000, Busse et al 2002, Warden et al 1999). Ultrasound has been historically considered to be a contraindication in these circumstances, though the exact reason for this remains unclear. Given the volume and quality of the published evidence, it would be entirely inappropriate for fractures to remain on the contraindication list.

NICE Guidance :

NICE provide numerous documents (freely available from their website - listed with the references) which identify the potential value of LIPS from both fresh fractures and those with delayed and no union. They concentrate on the established dose (1.5MHz; pulse 200 μ s; delivered at 20% duty cycle (1kHz); 30 mW cm⁻²; 20 minutes daily, usually as a patient delivered treatment (home based) with coupling gel as a contact medium between the treatment applicator and the skin.

Their 2010 review included a meta analysis of 1910 patients from one previous meta analysis (13 RCT's)(Busse et al, 2006) plus an additional 4 RCT's not included in the first meta analysis (Heckman et al, 1994; Emami et al, 1999; Leung et al, 2004; Ricardo, 2006), a comparative study (Coughlin et al, 2008) and a case series (Mayr et al, 2000). Full details are provided in the NICE document together with other research which they excluded for this work.

In their 2013 update, NICE appear to provide a paper supporting a specific machine (the Exogen device) though they do (in the detail) point out that this is not the only device available to deliver LIPUS. The guidance comes to the same general conclusion as the 2010 work, though there is some additional economic analysis which is insightful. "The case for adopting the Exogen ultrasound bone healing system to treat long bone fractures with non union (failure to heal after 9 months) is supported by the clinical evidence which shows high rates of fracture healing. The Exogen ultrasound bone healing system to treat long bone fractures with non union is associated with an estimated cost saving of £1164 per patient compared with current management, through avoiding surgery" (NICE 2013). The full paper (open access) clearly provides a more detailed analysis.

The Busse et al (2006) meta analysis (13 RCT's) reported an overall reduction in mean healing time of 34% (CI 21 - 44%) for patients receiving LIPUS compared with a sham treatment. The Heckman study (1994) involved tibial fractures, 33 patients treated with LIPUS and 34 in a sham group. They reported a significant increased rate of healing (96 days LIPUS group, 54 days sham group). The Leung et al (2004) study with 30 patients (16 LIPUS, 14 sham) with tibial fractures report an average time to full weight bearing of 9.3 weeks in the treated group and 15.5 weeks in the sham group (significant difference). The Coughlin et al (2008) study also involved 30 patients undergoing subtalar arthrodesis (15 LIPUS, 15 standard management) reported a significant difference in the number of patients healed at 9 weeks - 63% in the LIPUS group compared with 43% in the standard management group.

The Mayr et al (2000) review (case series) involved 1317 patients all of whom received LIPUS and an 89% overall healing rate, subdivided into 91% mean healing rate for the delayed unions and 86% for the non unions.

Some of these studies are considered in further detail below. The point here is that the NICE analysis of fracture healing rates from the available evidence is totally coincident with my own work. The NICE analysis also includes sections on return to function, safety and infection. NICE do state that although the data was derived from RCT's, some was of poor quality (low patient numbers, lack of blinding, publication bias).

The NICE conclusions (phrased differently for the patient guidance and the 'medical' guidance suggests that this treatment may provide significant benefit for patients with non union and delayed healing fractures in whom surgical intervention may be avoided and recovery of limb function may be accelerated. It is advised that non union and delayed healing long bone fractures, particularly of the tibia would be most likely to benefit from this treatment. It is considered that this treatment had the potential to be cost saving compared with standard management. Additionally, it is suggested that this treatment may be of some benefit in patients with fresh fractures, though there were concerns with regards the cost implications.

Clinical Trial Information

A recent systematic review and meta-analysis (Busse et al 2002) (as reported in the NICE section above) has carefully considered the evidence in respect to the effect of low intensity pulsed ultrasound on the time to fracture healing. They conclude that the evidence from randomised trials where the data could be pooled (3 studies, 158 fractures) that the time to fracture healing was significantly reduced in the ultrasound treated groups than in the control groups and the mean difference in healing time was 64 days.

Warden et al (1999) published a review paper concluded that from animal and human studies, the use of ultrasound could accelerate the rate of fracture repair by a factor of 1.6.

Heckman et al (1994) demonstrated a 38% reduction in the healing time for tibial fractures using a LIPUS device whilst Kristiansen et al (1997) demonstrated a 30% acceleration in healing for fractures of the radius.

Jensen (1998) identifies the beneficial effects of ultrasound in the treatment (as opposed to the diagnosis) of stress fractures with an overall success rate of 96%. The report fails to identify all relevant data for consideration and must therefore be considered with some caution in terms of 'quality evidence'.

Mayr et al (2000) report a series of outcomes when using low intensity pulsed ultrasound for patients with delayed unions (n=951) and non unions (n=366). The overall success rate for the delayed unions was 91% for the delayed and 86% for the non unions.

The authors undertook an interesting stratified analysis of their patients, and identified that those who were using non steroidal anti inflammatory drugs, calcium channel blockers or steroids had a less favourable outcome, a finding that could be considered to be consistent with several research publications that have tried to identify the mechanism by which the ultrasound could bring about

fracture healing acceleration and other wider research concerning the adverse influence of NSAID's on tissue repair (e.g. Tsai et al 2004, Evans & Butcher 2004).

A more recent paper (Rutten et al 2007) demonstrated a 73% union rate in their group of tibial non unions (n=71 patients) which is clearly much better than the most optimistic spontaneous healing rate in this group (usually cited at between 5 and 30%).

The use of such low doses has been shown to result in non significant increases in tissue temperature. **Using higher ultrasound doses could have an adverse effect on the fracture healing process** and the low intensity pulsed system is considered to be effective and safe for this patient group. Reher et al (1997) demonstrated a stimulative effect at low dose (0.1 W cm⁻²) whilst an inhibitory effect at a higher dose (1 – 2 W cm⁻²). Chang et al (2002) demonstrated that the effect of low intensity pulsed ultrasound in these circumstances was achieved by non thermal mechanisms rather than as a phenomenon secondary to thermal effects.

Both Tis et al (2002) and Sakurakichi et al (2004) have evaluated the use of ultrasound as a component of treatment (in an animal model) during distraction osteogenesis, and both have demonstrated significant benefits. Cook et al (2001) have demonstrated similar benefits following spinal fusion surgery and Tanzer et al (2001) have shown that the use of ultrasound in combination with porous intramedullary implants is also beneficial. There are many other studies concerning the use of US and bone repair, but essentially the published work shows a consistent benefit, and the use of low intensity pulsed ultrasound for patients with bone related disorders, including normally healing fractures, stress fractures, delayed and non unions and as a post surgical intervention should be considered positively.

One study (Schortinghuis et al 2004) that employed the SAFHS ultrasound system yet failed to demonstrate a significant effect (following deliberate bone injury – rat model) is probably related to the additional inclusion of a PTFE membrane – a GoreTex® like material). This would almost certainly not enable adequate ultrasound energy transmission due to the porous nature of the material, and the consequent air trapping, leading to ultrasound energy reflection.

The Warden et al (1999) paper provides a useful review and another useful review of this field can be found in Pounder and Harrison (2008).

Recent Evidence

Since initially composing this page, there have been a plethora of papers and reviews published concerning the use of LIPUS applications with fresh fractures, delayed and non-unions - in fact I now have over 500 such papers in my database - and I am pretty sure that this is not a complete list.

I have identified (below) some of the key papers and reviews since 2020 for those who want to catch up with the current state of the art. The reviews will provide a swift access of many original RCT and clinical studies

Reviews

Yang, J. et al (2022) Efficacy of adjuvant treatment for fracture nonunion/delayed union: a network meta-analysis of randomized controlled trials *BMC Musculoskeletal Disorders* 23(1): 481

This review considers multiple interventions for fracture delayed / non-union - including LIPUS - which as an intervention, is supported

Palanisamy, P. et al (2022) Low-Intensity Pulsed Ultrasound Stimulation for Bone Fractures Healing: A Review *J Ultrasound Med* 41(3): 547

This review considers clinical effectiveness together with mechanisms of action - with fresh fractures, delayed and non-unions. The authors conclude "Overall, LIPUS has shown positive results on bone fracture healing through the molecular, biological, and biomechanical changes around the fracture site. It has been proven to accelerate the bone formation in fresh fractures, delayed unions, nonunions, and distraction osteogenesis. LIPUS treatment is recommended as a safe therapy when compared to existing fracture treatments, and can be used as an adjunctive therapy to accelerate the bone healing process for fresh fractures, delayed fractures, and nonunions."

Elmajee, M. et al (2022) The perceptions of clinicians using low-intensity pulsed ultrasound (LIPUS) for orthopaedic pathology: A national qualitative study *Injury*

This review considers the results of a (UK) survey considering LIPUS use for fracture healing. The authors conclude "LIPUS technology may have a significant role to play in the treatment of orthopaedic fracture related pathology. Regular users perceived the technology to be cost-effective and efficacious."

Puts, R. et al (2021) Pulsed ultrasound for bone regeneration - outcomes and hurdles in the clinical application: a systematic review *Eur Cell Mater* 41: 281

This review tackles some of the controversies that have emerged in the more recent published literature - and some of the apparent discrepancies in results and conclusions reached.

Leighton, R. et al (2021) Low intensity pulsed ultrasound (LIPUS) use for the management of instrumented, infected, and fragility non-unions: a systematic review and meta-analysis of healing proportions *BMC Musculoskeletal Disorders* 22(1): 532

Nice review which considers 'problematic' fracture healing based on N=29 studies. The authors conclude "This study has provided a thorough overview of the current literature on LIPUS treatment for instrumented, infected, and fragility fracture non-unions. The healing rates for non-unions in these subgroups were comparable to healing rates observed with LIPUS use in general non-union literature. LIPUS treatment should be considered as a conservative non-surgical treatment option to potentially reduce the socioeconomic impact and improve the quality of life of these unfortunate patients."

Harrison, A. & Alt, V. (2021) Low-intensity pulsed ultrasound (LIPUS) for stimulation of bone healing - A narrative review *Injury* 52 Suppl 2: S91

The broadly scoped review also tackles some of the controversies and mixed results - especially regarding poor results with internally fixed fractures.

Majeed, H. et al (2020) Clinical and patient-reported outcomes following Low Intensity Pulsed Ultrasound (LIPUS, Exogen) for established post-traumatic and post-surgical nonunion in the foot and ankle *Foot Ankle Surg* 26(4): 405

There are several papers which have looked at the use of LIPUS in the foot and ankle - this review provides a useful overview. The authors conclusions are positive "Exogen for established nonunion in the foot and ankle is a safe, valuable and economically viable clinical option as an alternative to revision surgery. We observed better results in the fracture and midfoot/forefoot groups and relatively poorer results in the hindfoot fusion group."

Elvey, M. H. et al (2020) The use of low-intensity pulsed ultrasound in hand and wrist nonunions *J Plast Surg Hand Surg* 54(2): 101

Many studies (and reviews) only really consider lower limb fractures and unions. This paper specifically looks at wrist and hand issues. While the healing rates may not be as profound as for the lower limb, the treatment still has positive effects and clinical benefits when surgery is not a viable option.

Berber, R. et al (2020) Low Intensity Pulsed Ultrasound Therapy (LIPUS): A review of evidence and potential applications in diabetics *J Clin Orthop Trauma* 11(Suppl 4): S500

Interesting take on the classical review - specifically looking at LIPUS use for fractures in patients with diabetes. Actually includes both animal and human studies but provides some useful insights.

I will not go on to list all the non-review papers (would get somewhat arduous) but sure that if I can find them, then so can the interested reader

Summary and Conclusion

There is good lab, cell, animal and clinical (RCT and other) evidence to support the use of LIPUS in patients with fractures. It has demonstrated benefit for fresh fractures, those with delayed healing and those with established non union. In current clinical practice, it is most commonly employed for those with fracture healing problems (though in elite sport for example, it is routinely used on most, if not all fractures given that speed of healing and rapid return to sport is a time critical activity).

The intervention is supported by the NICE guidance, and thus would constitute a recognised 'evidence based' treatment. It is not routinely incorporated into therapy practice, though it is suggested that this position should change in the near future. The treatment need not involve 'therapy time' beyond setting up the treatment and teaching the patient how to manage the device. The treatment is best

delivered using a home based, patient delivery system. The effective treatment dose is known and well established (summarised as 1.5MHz; 0.03 W cm⁻²; 20% duty cycle at 1kHz; 20 minutes; daily).

There is currently not enough evidence to support the use of a 'regular' therapy ultrasound machine to deliver this treatment. Not only are most therapy machines completely unable to deliver the evidenced therapy, the treatment needs to be delivered on a daily basis, and this therefore may be an ineffective use of a therapy machine which is 'in demand' in a department or clinic.

References :

Aiyegbusi, A., F. Duru, et al. (2012). "The healing of acute tendon injuries: effects of intrasound therapy and low intensity pulsed ultrasound." *Journal of Bodywork and Movement Therapies* 16(4): 524-524.

Busse, J. W., M. Bhandari, et al. (2002). "The effect of low-intensity pulsed ultrasound therapy on time to fracture healing: a meta-analysis." *CMAJ* 166(4): 437-41.

Chang, W. H., J. S. Sun, et al. (2002). "Study of thermal effects of ultrasound stimulation on fracture healing." *Bioelectromagnetics* 23(4): 256-63.

Cook, S. D., S. L. Salkeld, et al. (2001). "Low-intensity pulsed ultrasound improves spinal fusion." *The Spine Journal* 1: 246-254.

Evans, C. E. and C. Butcher (2004). *Journal of Bone and Joint Surgery* 86-B(3): 444-449.

Heckman, J. D., J. P. Ryaby, et al. (1994). "Acceleration of tibial fracture-healing by non-invasive, low-intensity pulsed ultrasound." *J Bone Joint Surg Am* 76(1): 26-34.

Jensen, J. E. (1998). "Stress fracture in the world class athlete: a case study." *Med Sci Sports Exerc* 30(6): 783-7.

Johns, L. D., S. J. Straub, et al. (2007). "Analysis of effective radiating area, power, intensity, and field characteristics of ultrasound transducers." *Arch Phys Med Rehabil* 88(1): 124-129.

Kinami, Y., T. Noda, et al. (2013). "Efficacy of low-intensity pulsed ultrasound treatment for surgically managed fresh diaphyseal fractures of the lower extremity: multi-center retrospective cohort study." *J Orthop Sci* 18(3): 410-418.

Kristiansen, T. K., J. P. Ryaby, et al. (1997). "Accelerated healing of distal radial fractures with the use of specific, low-intensity ultrasound. A multicenter, prospective, randomized, double-blind, placebo-controlled study." *J Bone Joint Surg Am* 79(7): 961-73.

Lerner, A., H. Stein, et al. (2004). "Compound high-energy limb fractures with delayed union: our experience with adjuvant ultrasound stimulation (exogen)." *Ultrasonics* 42: 915-917.

Mayr, E., V. Frankel, et al. (2000). "Ultrasound--an alternative healing method for nonunions?" *Arch Orthop Trauma Surg* 120(1-2): 1-8.

Pounder, N. M. and A. J. Harrison (2008). "Low intensity pulsed ultrasound for fracture healing: a review of the clinical evidence and the associated biological mechanism of action." *Ultrasonics* 48(4): 330-8.

Reher, P., N. I. Elbeshir el, et al. (1997). "The stimulation of bone formation in vitro by therapeutic ultrasound." *Ultrasound Med Biol* 23(8): 1251-8.

Reher, P., M. Harris, et al. (2002). "Ultrasound stimulates nitric oxide and prostaglandin E2 production by human osteoblasts." *Bone* 31(1): 236-41.

Rutten, S., P. A. Nolte, et al. (2007). "Use of low-intensity pulsed ultrasound for posttraumatic nonunions of the tibia: a review of patients treated in the Netherlands." *J Trauma* 62(4): 902-8.

Sakurakichi, K., H. Tsuchiya, et al. (2004). "Effects of timing of low-intensity pulsed ultrasound on distraction osteogenesis." *J Orthop Res* 22: 395-403.

Schortinghuis, J., J. L. Rubenb, et al. (2004). "Therapeutic ultrasound to stimulate osteoconduction A placebo controlled single blind study using e-PTFE membranes in rats." *Archives of Oral Biology* 49: 413-420.

Tanzer, M., S. Kantor, et al. (2001). "Enhancement of bone growth into porous intramedullary implant using non-invasive low intensity ultrasound." *J Orthop Res* 19: 195-199.

ter Haar, G. (1999). "Therapeutic Ultrasound." *Eur J Ultrasound* 9: 3-9.

Tis, J. E., R. H. Meffert, et al. (2002). "The effect of low intensity pulsed ultrasound applied to rabbit tibiae during the consolidation phase of distraction osteogenesis." *J Orthop Res* 20: 793-800.

Tsai, W.-C., F.-T. Tang, et al. (2004). "Ibuprofen inhibition of tendon cell proliferation and upregulation of the cyclin kinase inhibitor p21CIP1." *Journal of Orthopaedic Research* 22(3): 586-591.

Warden, S., K. Bennell, et al. (1999). "Can conventional therapeutic ultrasound units be used to accelerate fracture repair?" *Phys Ther Rev* 4: 117-126.

Warden, S. J., J. M. Favaloro, et al. (2001). "Low-intensity pulsed ultrasound stimulates a bone-forming response in UMR-106 cells." *Biochem Biophys Res Commun* 286(3): 443-50.

LIPUS Mechanisms

Claes, L. and B. Willie (2007). "The enhancement of bone regeneration by ultrasound." *Prog Biophys Mol Biol* 93(1-3): 384-398.

Della Rocca, G. J. (2009). "The science of ultrasound therapy for fracture healing." *Indian J Orthop* 43(2): 121-126.

Ebisawa, K., K. Hata et al (2004). "Ultrasound enhances transforming growth factor beta-mediated chondrocyte differentiation of human mesenchymal stem cells." *Tissue Eng* 10(5-6): 921-929.

Freeman, T. A., P. Patel et al (2009). "Micro-CT analysis with multiple thresholds allows detection of bone formation and resorption during ultrasound-treated fracture healing." *J Orthop Res* 27(5): 673-679.

Fung, C. H., W. H. Cheung, et al. (2012). "Effects of Different Therapeutic Ultrasound Intensities on Fracture Healing in Rats." *Ultrasound Med Biol* 38(5): 745-752.

Jingushi, S., K. Mizuno et al (2007). "Low-intensity pulsed ultrasound treatment for postoperative delayed union or nonunion of long bone fractures." *J Orthop Sci* 12(1): 35-41.

Jingushi, S. (2009). "[Bone fracture and the healing mechanisms. Fracture treatment by low-intensity pulsed ultrasound]." *Clin Calcium* 19(5): 704-708.

Kokubu, T., N. Matsui et al (1999). "Low intensity pulsed ultrasound exposure increases prostaglandin E2 production via the induction of cyclooxygenase-2 mRNA in mouse osteoblasts." *Biochem Biophys Res Commun* 256(2): 284-287.

Lai, C. H., S. C. Chen et al (2010). "Effects of low-intensity pulsed ultrasound, dexamethasone/TGF-beta1 and/or BMP-2 on the transcriptional expression of genes in human mesenchymal stem cells: chondrogenic vs. osteogenic differentiation." *Ultrasound Med Biol* 36(6): 1022-1033.

Leung, K. S., W. H. Cheung et al (2004). "Low intensity pulsed ultrasound stimulates osteogenic activity of human periosteal cells." *Clin. Orthop. Rel. Res.*(418): 253-259.

Lu, H., L. Qin et al (2009). "Identification of genes responsive to low-intensity pulsed ultrasound stimulations." *Biochem Biophys Res Commun* 378(3): 569-573.

Naruse, K., Y. Mikuni-Takagaki et al (2009). "Therapeutic ultrasound induces periosteal ossification without apparent changes in cartilage." *Connect Tissue Res* 50(1): 55-63.

Naruse, K., H. Sekiya et al (2010). "Prolonged endochondral bone healing in senescence is shortened by low-intensity pulsed ultrasound in a manner dependent on COX-2." *Ultrasound Med Biol* 36(7): 1098-1108.

Nolte, P. A., J. Klein-Nulend et al (2001). "Low intensity ultrasound stimulates endochondral ossification in vitro." *J Orthop Res* 19: 301-307.

Padilla, F., R. Puts, et al. (2014). "Stimulation of bone repair with ultrasound: a review of the possible mechanic effects." *Ultrasonics* 54(5): 1125-1145.

Ryaby, J. T., J. Mathew et al (1991). *Electromagnetics in Biology and Medicine*. C. T. Brighton and S. R. Pollack. San Francisco, San Francisco Press.

Sant'Anna, E. F., R. M. Leven et al (2005). "Effect of low intensity pulsed ultrasound and BMP-2 on rat bone marrow stromal cell gene expression." J Orthop Res 23(3): 646-652.

Sena, K., R. M. Leven et al (2005). "Early gene response to low-intensity pulsed ultrasound in rat osteoblastic cells" Ultrasound in Medicine & Biology 31(5): 703-708.

Tang, C. H., R. S. Yang et al (2006). "Ultrasound stimulates cyclooxygenase-2 expression and increases bone formation through integrin, focal adhesion kinase, phosphatidylinositol 3-kinase, and Akt pathway in osteoblasts." Mol Pharmacol 69(6): 2047-2057.

Wang, F. S., Y. R. Kuo et al (2004). "Nitric oxide mediates ultrasound-induced hypoxia-inducible factor-1alpha activation and vascular endothelial growth factor-A expression in human osteoblasts." Bone 35(1): 114-123.

Warden, S. J. (2003). "A new direction for ultrasound therapy in sports medicine." Sports Med 33(2): 95-107.

Warden, S. J., R. K. Fuchs et al (2006). "Ultrasound produced by a conventional therapeutic ultrasound unit accelerates fracture repair." Physical Therapy 86(8): 1118-1127.

Web Resources :

NICE LIPUS data

There are several NICE documents available with regards the use of LIPUS for fracture healing. This page will make a useful start point, and other documents can be found via the links from here :

2010 :

<http://publications.nice.org.uk/low-intensity-pulsed-ultrasound-to-promote-fracture-healing-ipg374>

2013

<http://guidance.nice.org.uk/MTG12/Guidance/pdf/English>

LIPUS Manufacturer and Distributor pages

Exogen (Smith and Nephew) :

global.smith-nephew.com/master/EXOGEN_ULTRASOUND_BONE_HEALING_SYSTEM.htm

Osteotron (EMS Physio) :

www.emsphysio.co.uk/124_osteotron-iv.htm

Updated LIPUS information on :: www.electrotherapy.org/modality/ultrasound-for-fracture-healing